


QAL 3 Shewart Chart Summary Page

Instrument and Species	SPAN	ZERO
Line One Duty MIRFT - CO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line One Duty MIRFT - CO2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line One Duty MIRFT - HCl	Last Test Date 10/06/2026 Bottle Used Hydrogen Chloride (New) Bottle Expiry Date 31/10/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line One Duty MIRFT - N2O	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
	PASS	
Line One Duty MIRFT - NH3	Last Test Date 10/06/2026 Bottle Used Ammonia Bottle Expiry Date 04/02/2026	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
	PASS	
Line One Duty MIRFT - NO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line One Duty MIRFT - O2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025
		PASS
Line One Duty MIRFT - Propane	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
	PASS	
Line One Duty MIRFT - SO2	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS

QAL3 Report For CO from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : CO

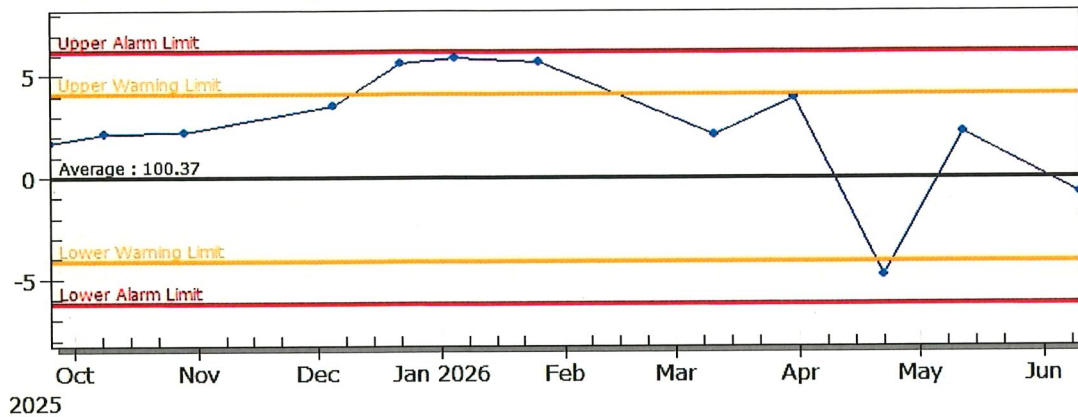

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : CO

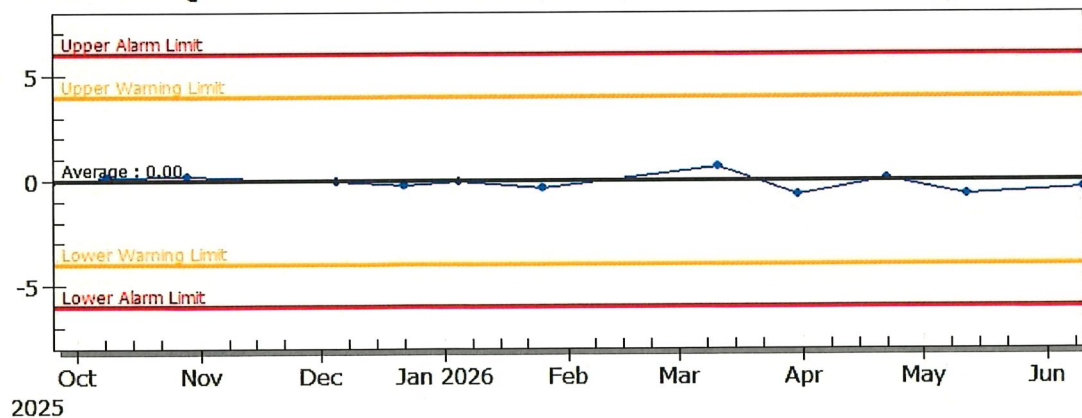


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For CO2 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : CO2

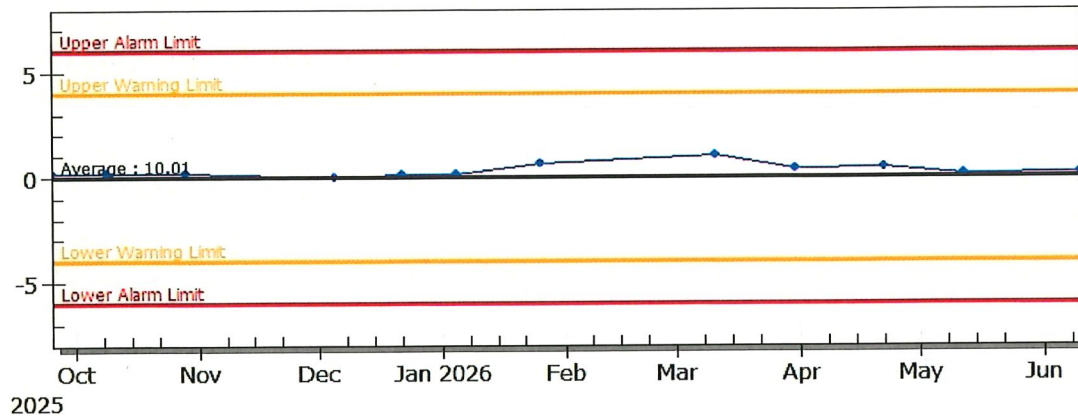

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : CO2

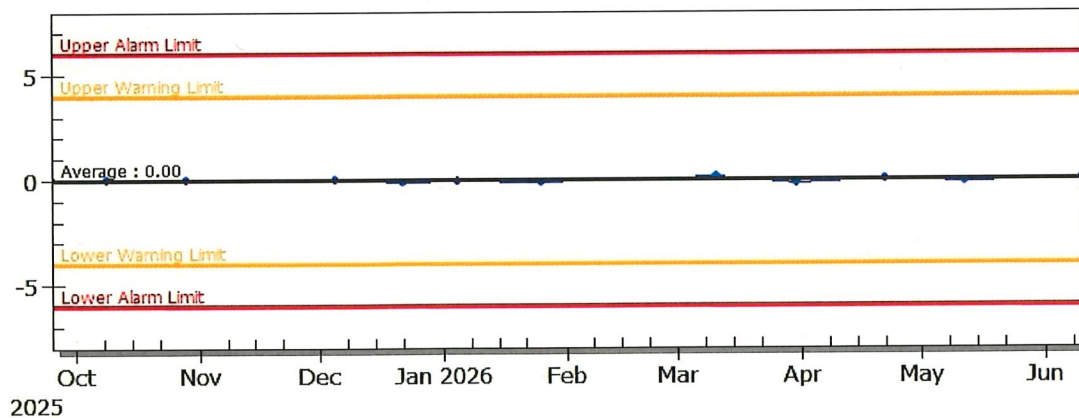


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For HCl from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : HCl

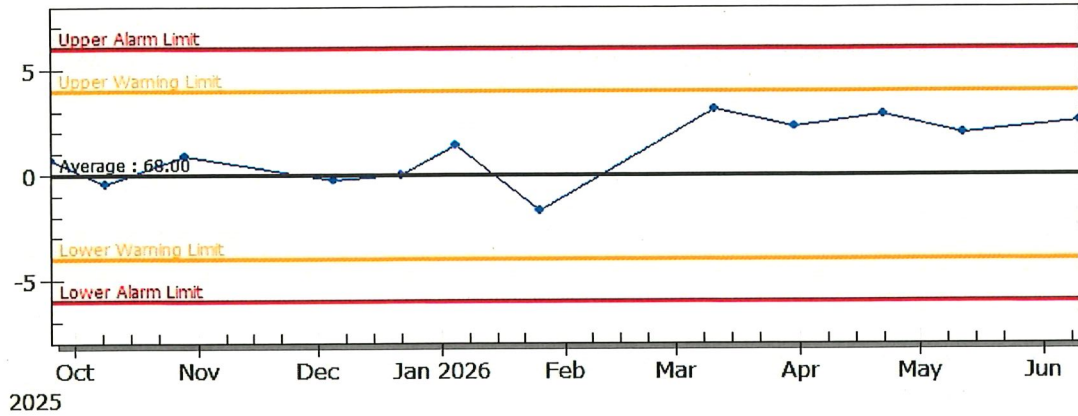

Last Test Date 10/06/2026 - Bottle Name Hydrogen Chloride (New) - Expiry Date 31/10/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : HCl

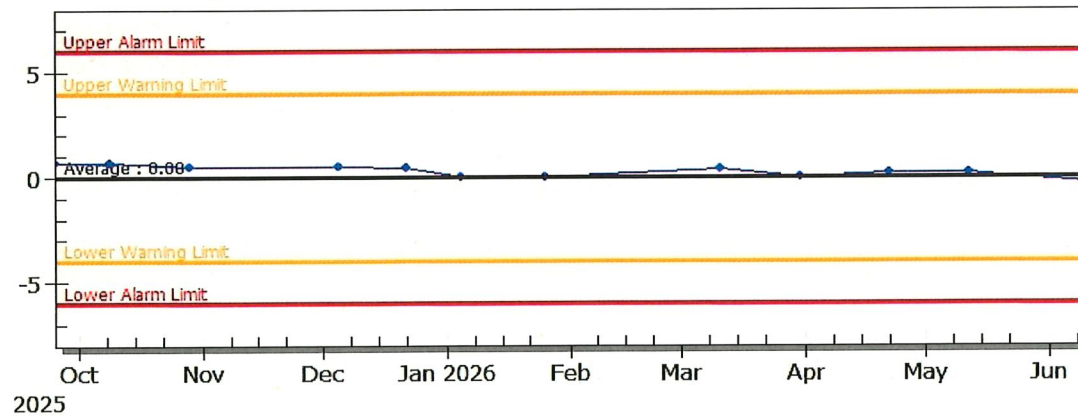


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For N2O from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : N2O

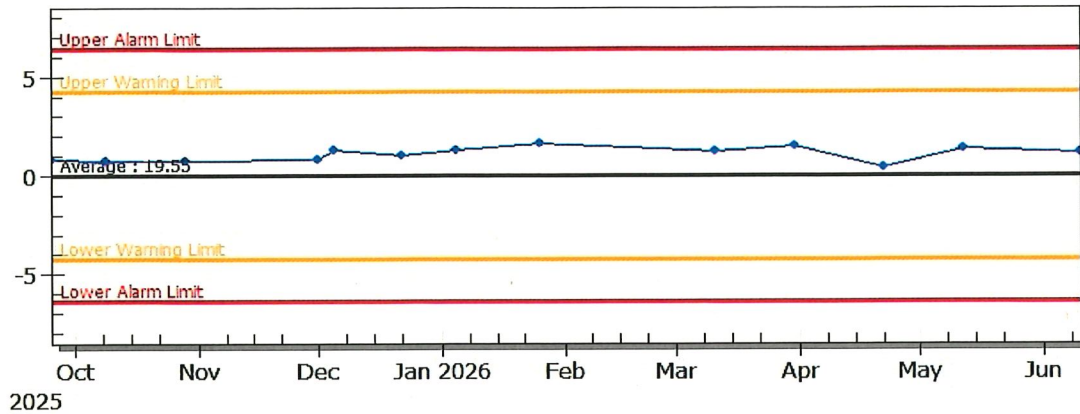

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : N2O

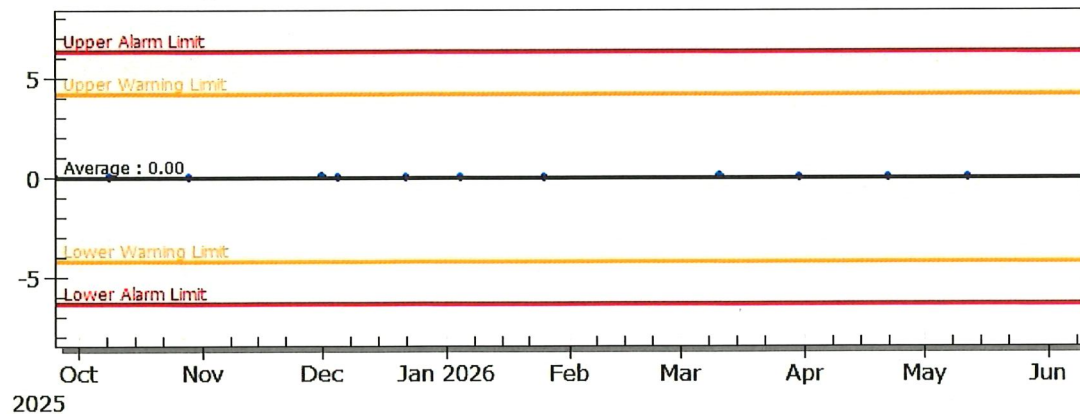


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NH3 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : NH3

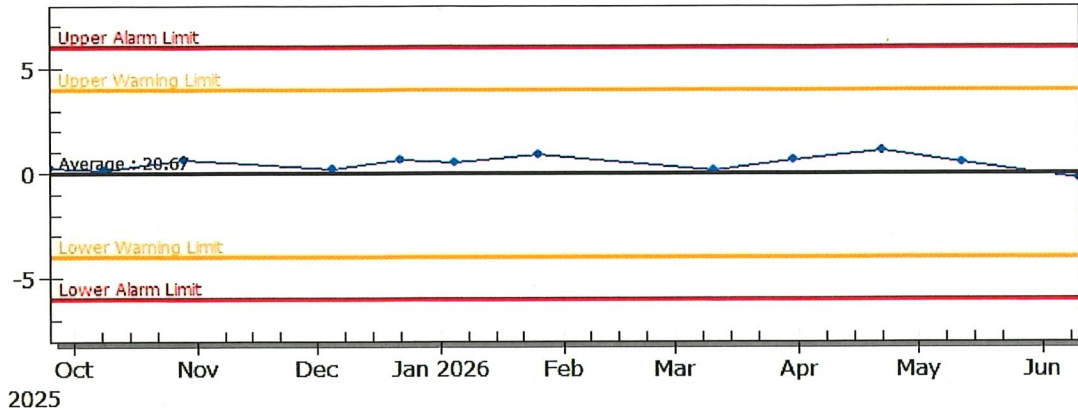

Last Test Date 10/06/2026 - Bottle Name Ammonia - Expiry Date 04/02/2026

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : NH3

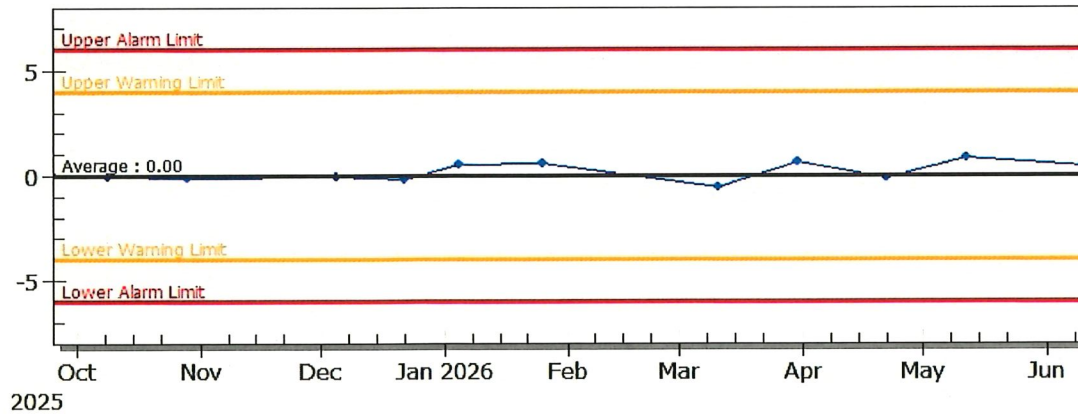


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NO from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : NO

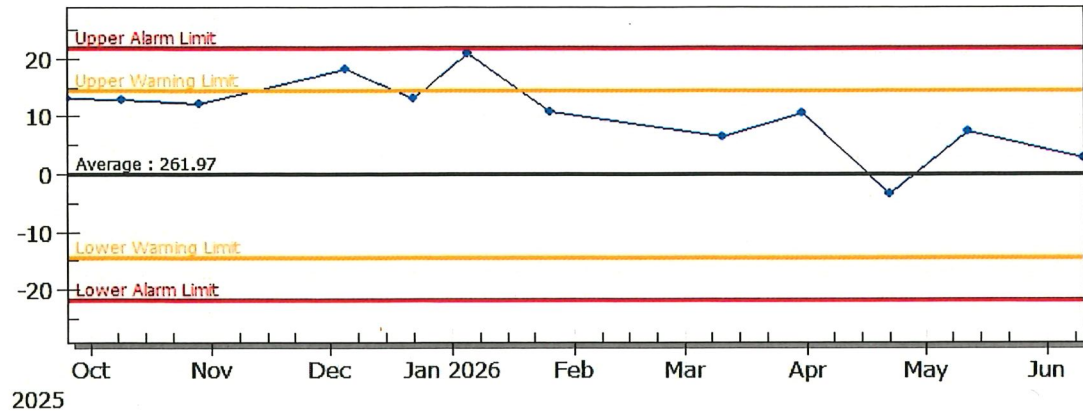

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : NO

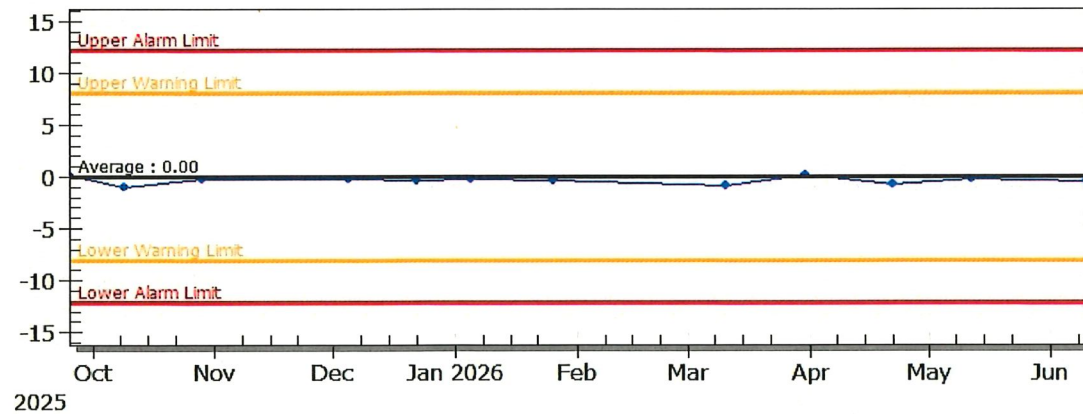


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For O2 from 25 September 2025 to 10 June 2026

EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : O2

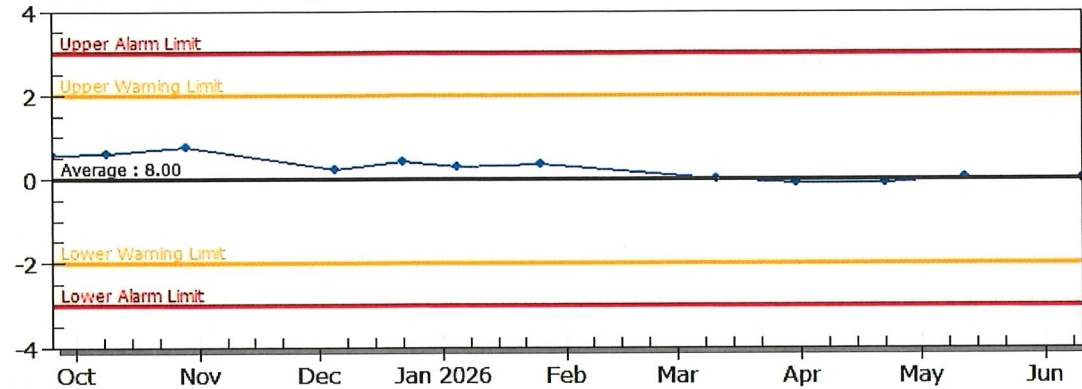


2025

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : O2

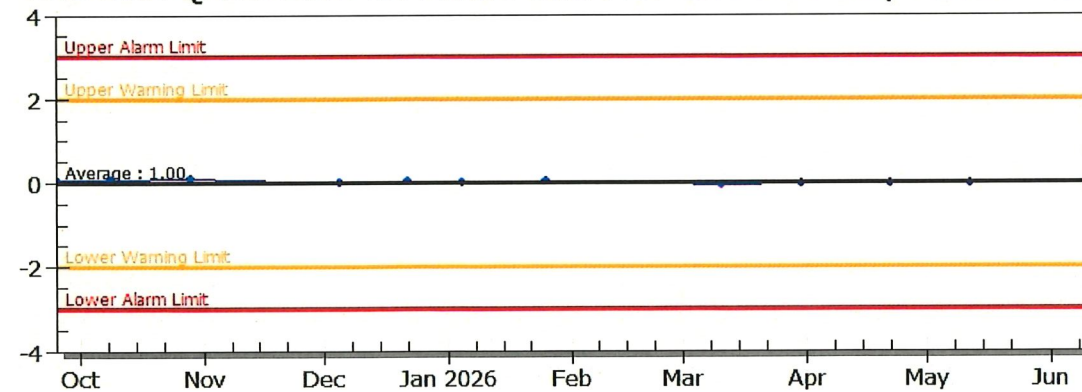


2025

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

QAL3 Report For Propane from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : Propane

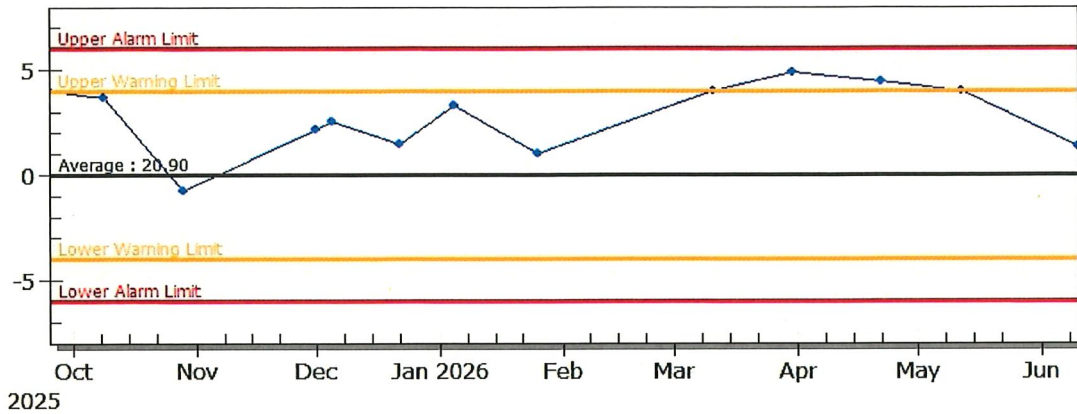

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : Propane

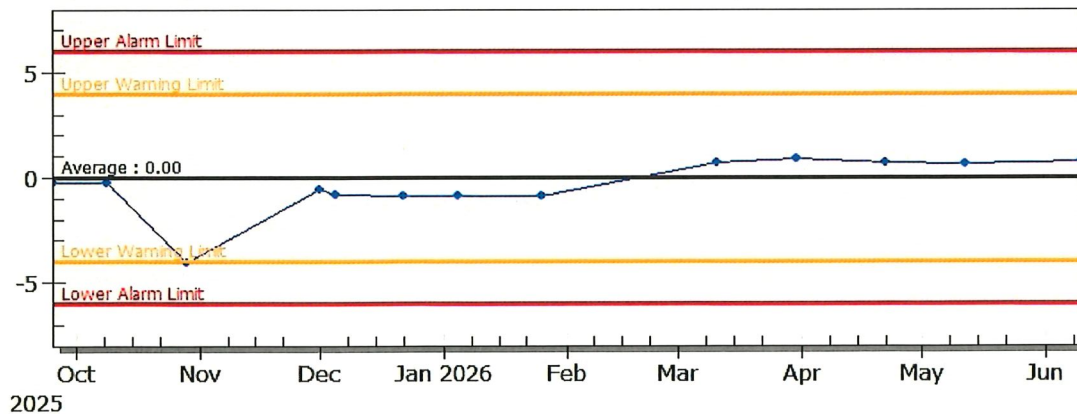


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For SO2 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line One Duty MIRFT : SO2

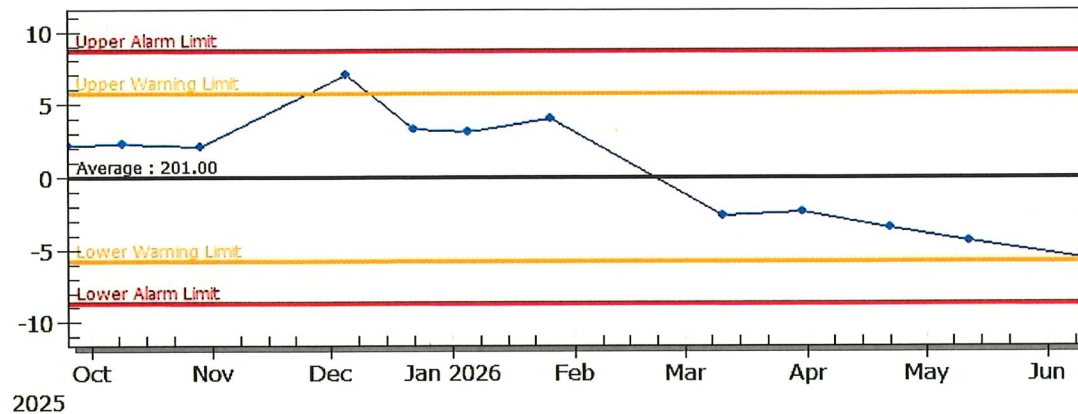

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line One Duty MIRFT : SO2

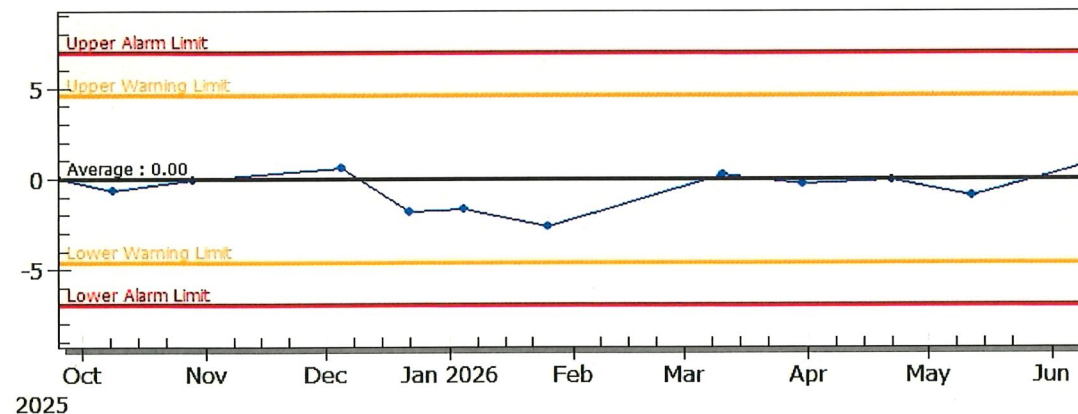

Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL 3 Shewart Chart Summary Page


Instrument and Species	SPAN	ZERO
Line Two Duty MIRFT - CO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 FAILURE	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - CO2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - HCl	Last Test Date 10/06/2026 Bottle Used Hydrogen Chloride (New) Bottle Expiry Date 31/10/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - N2O	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - NH3	Last Test Date 10/06/2026 Bottle Used Ammonia Bottle Expiry Date 04/02/2026 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - NO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - O2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 PASS
Line Two Duty MIRFT - Propane	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Line Two Duty MIRFT - SO2	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS

Reasons for Failures/Warnings

Line Two Duty MIRFT - CO - Span Test - Single Point Above the Alarm Limit (10 June 2026)

QAL3 Report For CO from 24 September 2025 to 10 June 2026

EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : CO

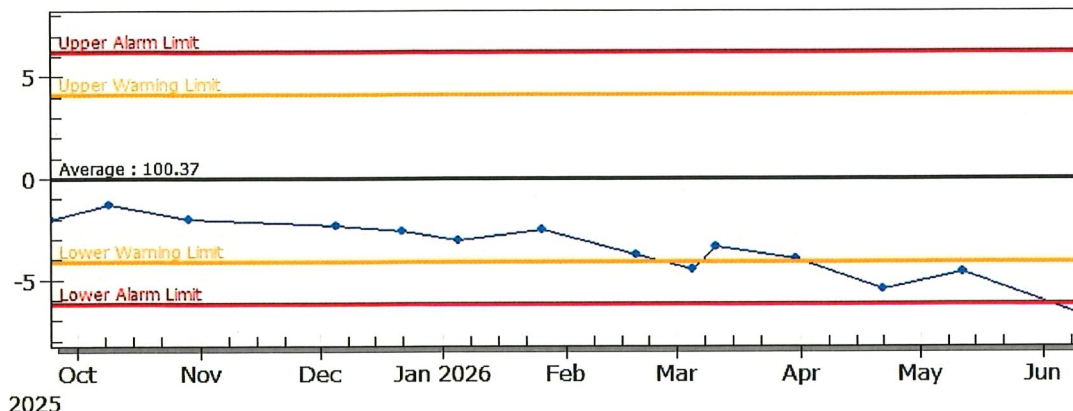


Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Has Failures and/or Warnings

Span Test - Single Point Above the Alarm Limit (10 June 2026)

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : CO

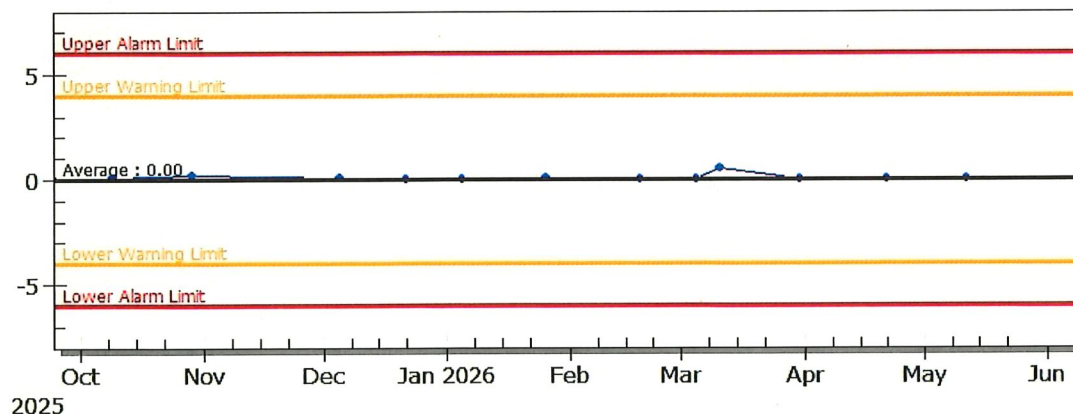


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For CO2 from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : CO2

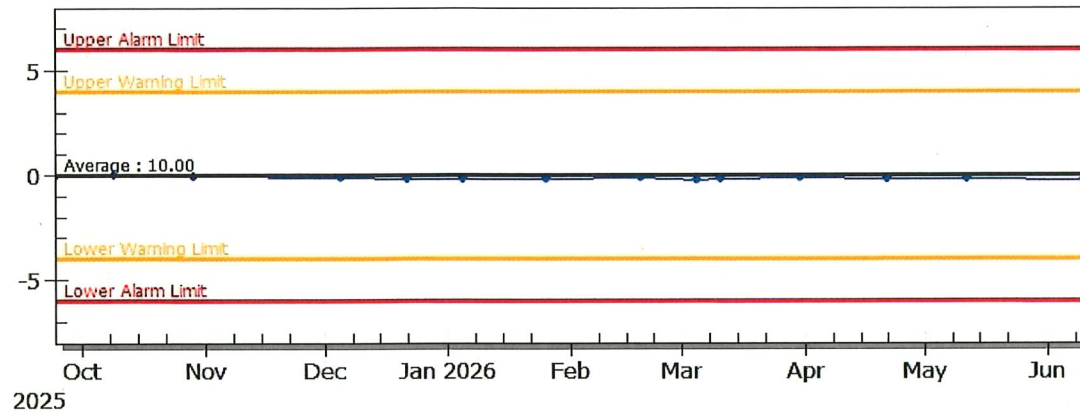

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : CO2

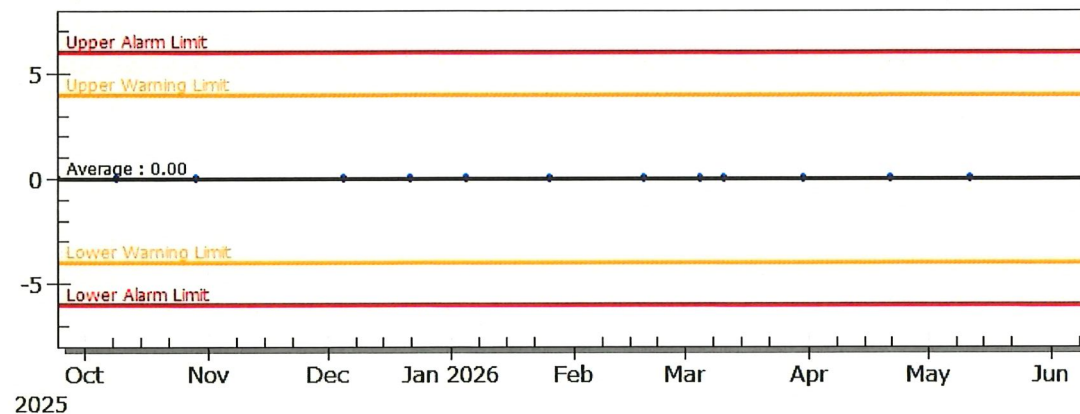


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For HCI from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : HCI

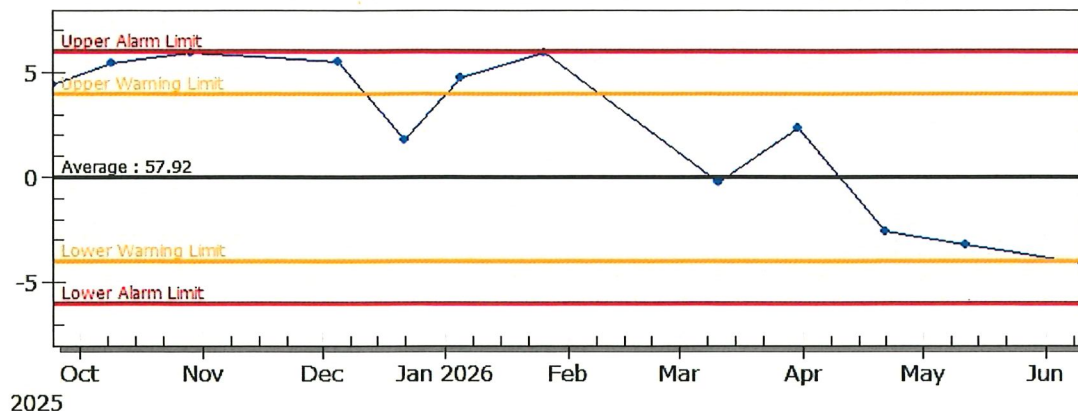

Last Test Date 10/06/2026 - Bottle Name Hydrogen Chloride (New) - Expiry Date 31/10/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : HCI

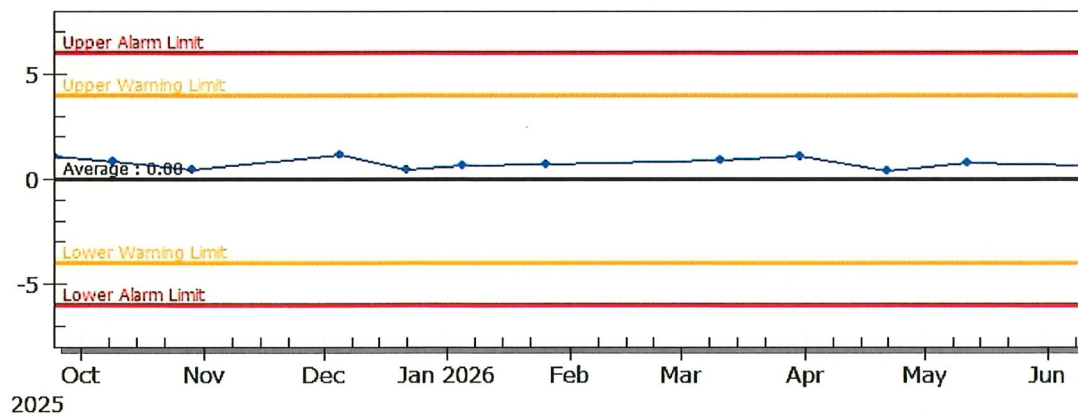


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For N2O from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : N2O

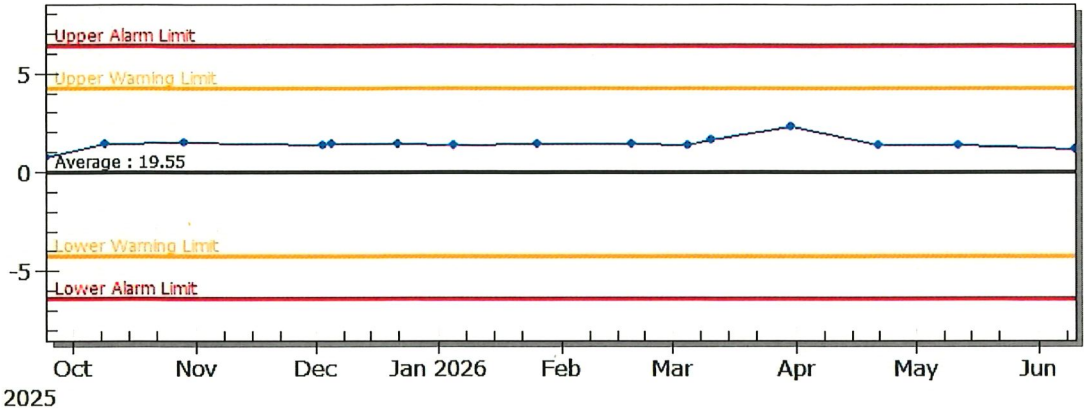

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : N2O

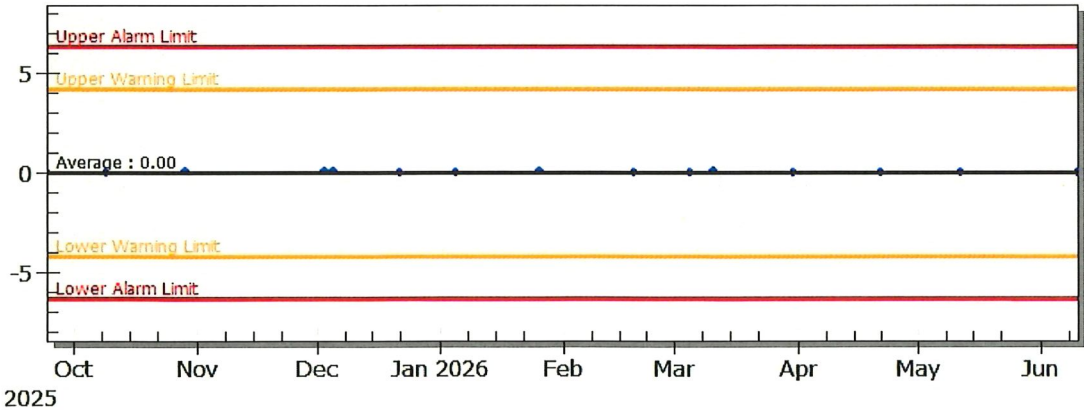


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NH3 from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : NH3

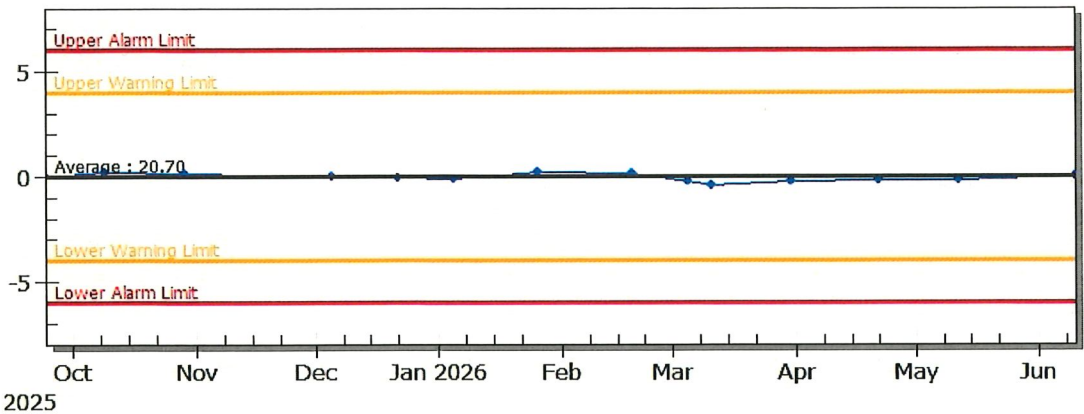

Last Test Date 10/06/2026 - Bottle Name Ammonia - Expiry Date 04/02/2026

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : NH3

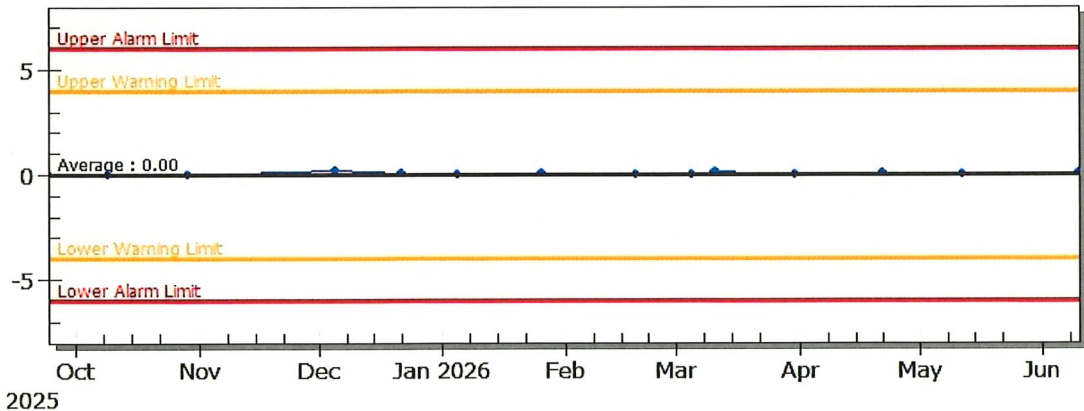


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NO from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : NO

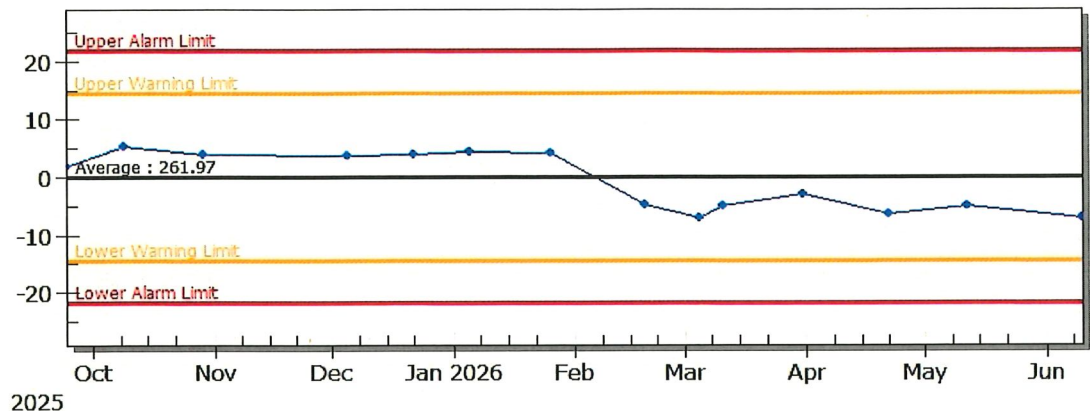

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : NO

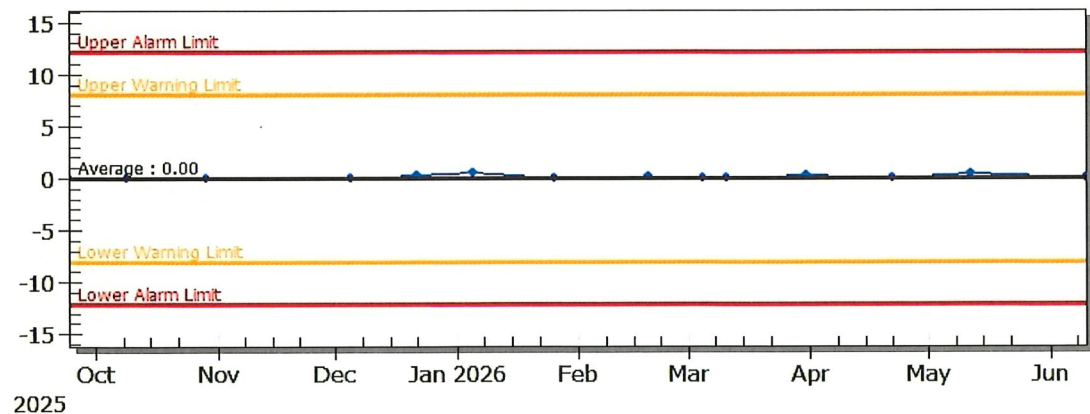


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For O2 from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : O2

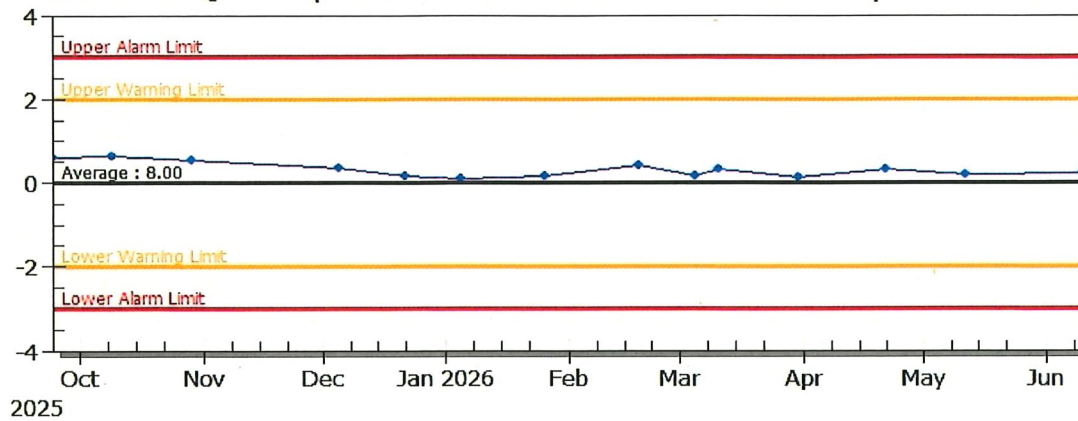

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : O2

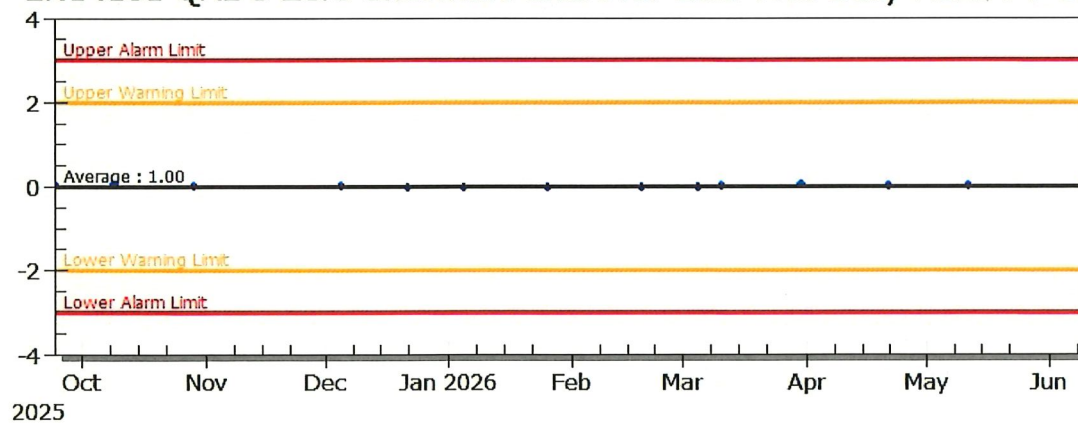


Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

QAL3 Report For Propane from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : Propane

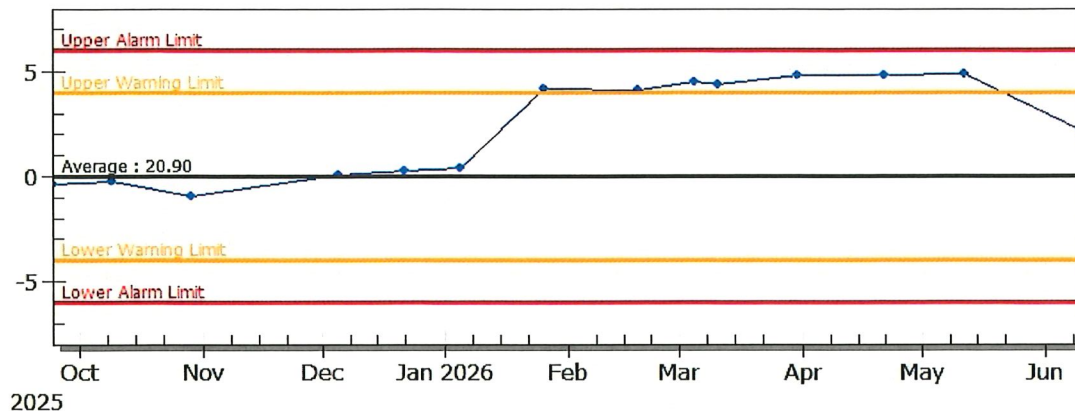

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : Propane

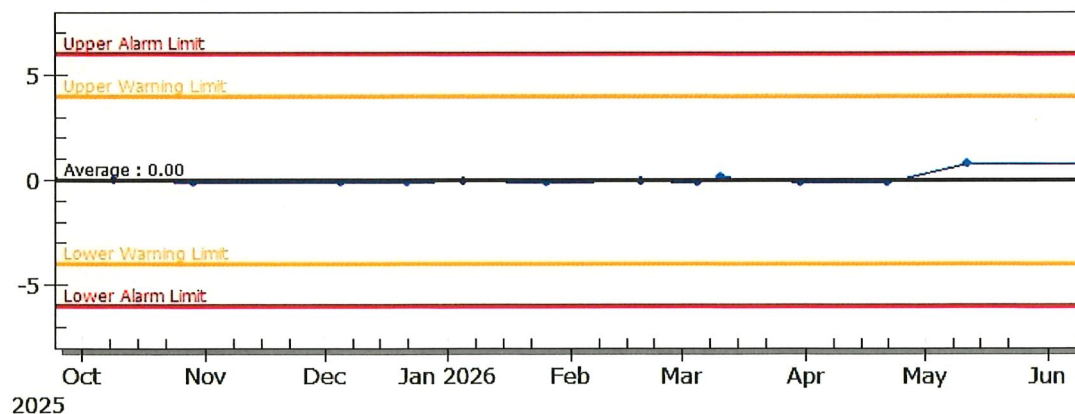


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For SO2 from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : SO2

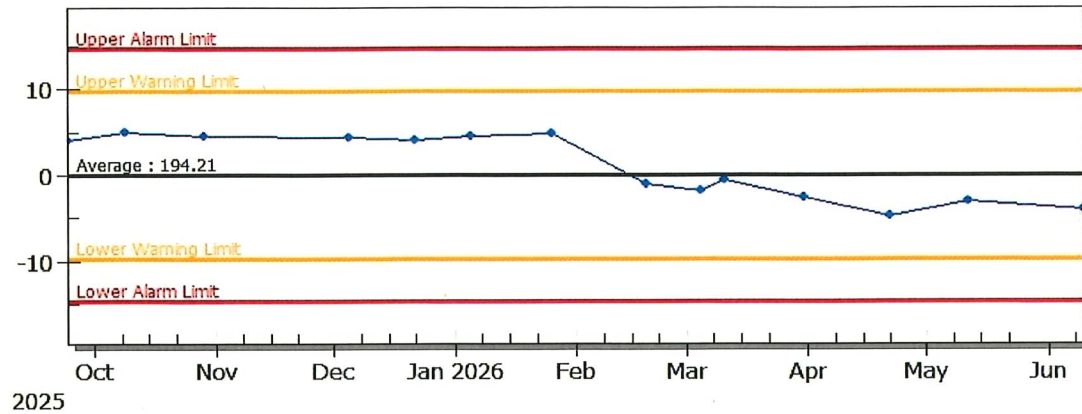

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : SO2

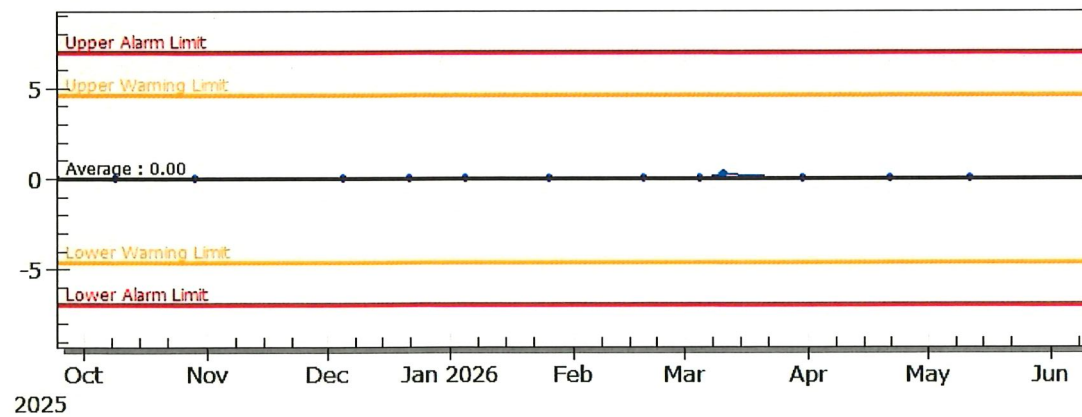

Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030


Test Passed

QAL 3 Shewart Chart Summary Page

Instrument and Species	SPAN	ZERO
Line Two Duty MIRFT - CO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS

QAL3 Report For CO from 24 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Line Two Duty MIRFT : CO

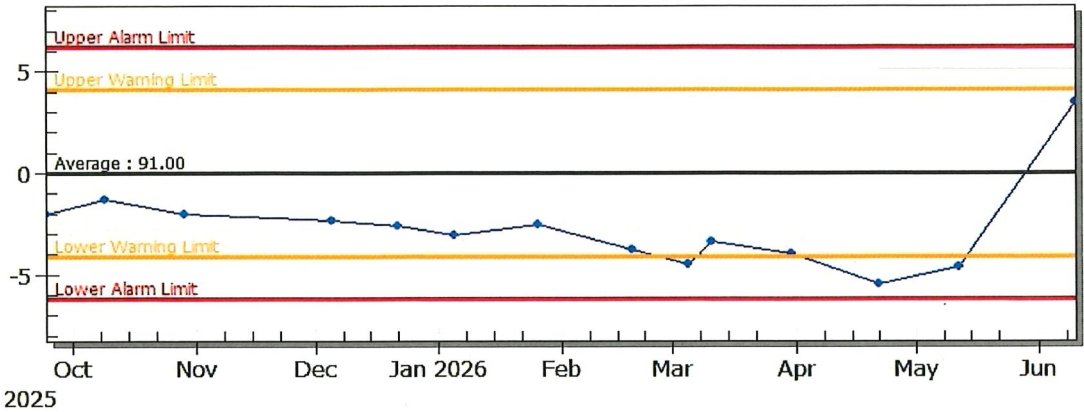

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Line Two Duty MIRFT : CO

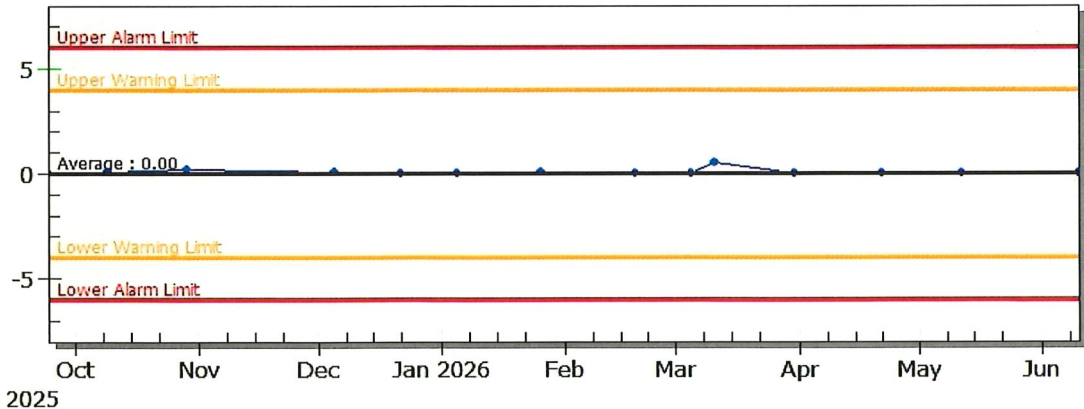

Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL 3 Shewart Chart Summary Page


Instrument and Species	SPAN	ZERO
Standby MIRFT - CO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - CO2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - HCl	Last Test Date 10/06/2026 Bottle Used Hydrogen Chloride (New) Bottle Expiry Date 31/10/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - N2O	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - NH3	Last Test Date 10/06/2026 Bottle Used Ammonia Bottle Expiry Date 04/02/2026 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - NO	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - O2	Last Test Date 10/06/2026 Bottle Used CO2/O2 Bottle Expiry Date 20/12/2027 PASS	Last Test Date 29/10/2025 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 PASS
Standby MIRFT - Propane	Last Test Date 10/06/2026 Bottle Used N2O / O2 / Propane Bottle Expiry Date 06/09/2025 FAILURE	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS
Standby MIRFT - SO2	Last Test Date 10/06/2026 Bottle Used CO/SO2/NO Bottle Expiry Date 15/08/2028 PASS	Last Test Date 10/06/2026 Bottle Used Nitrogen Bottle Expiry Date 25/12/2030 PASS

Reasons for Failures/Warnings

Standby MIRFT - Propane - Span Test - Single Point Above the Alarm Limit (10 June 2026)

QAL3 Report For CO from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : CO

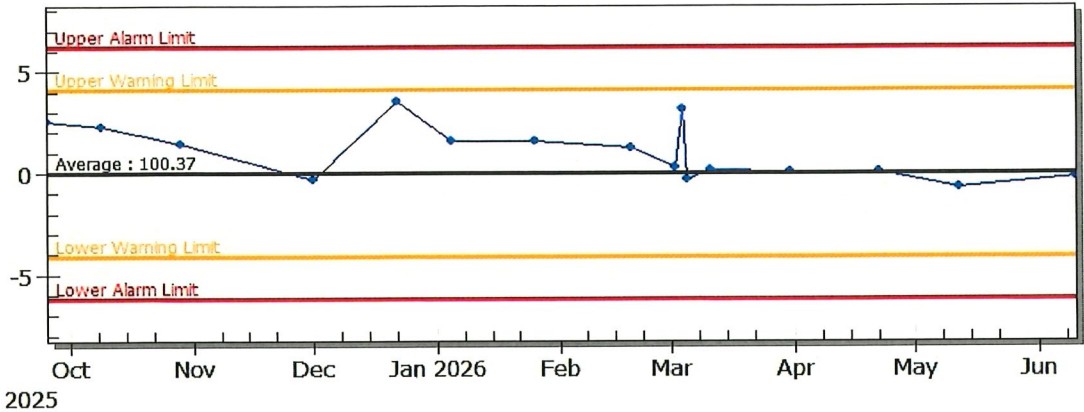

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : CO

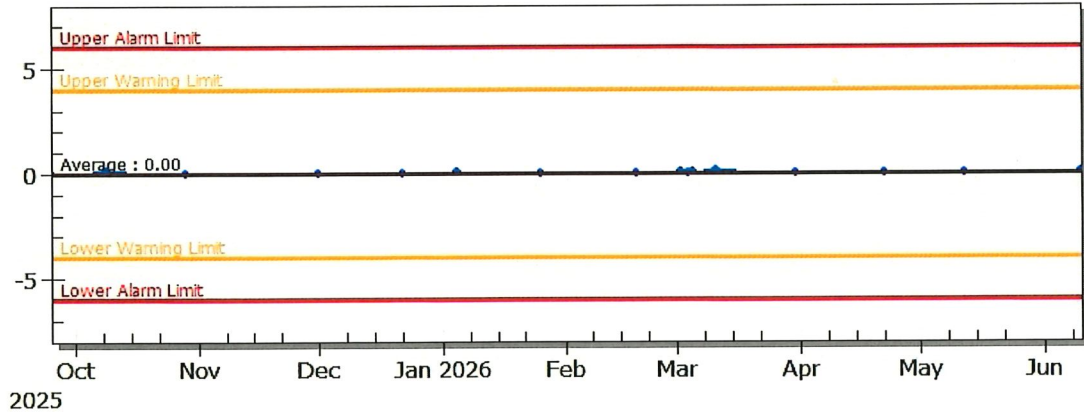


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For CO2 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : CO2

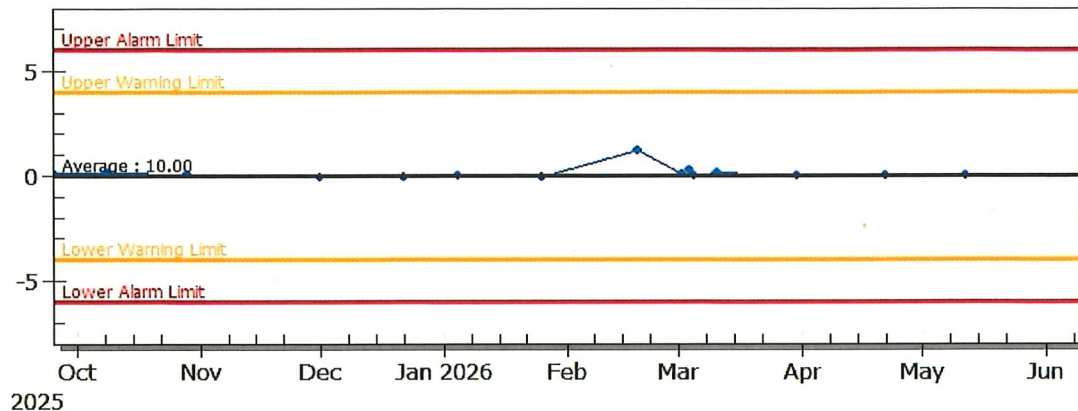

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : CO2

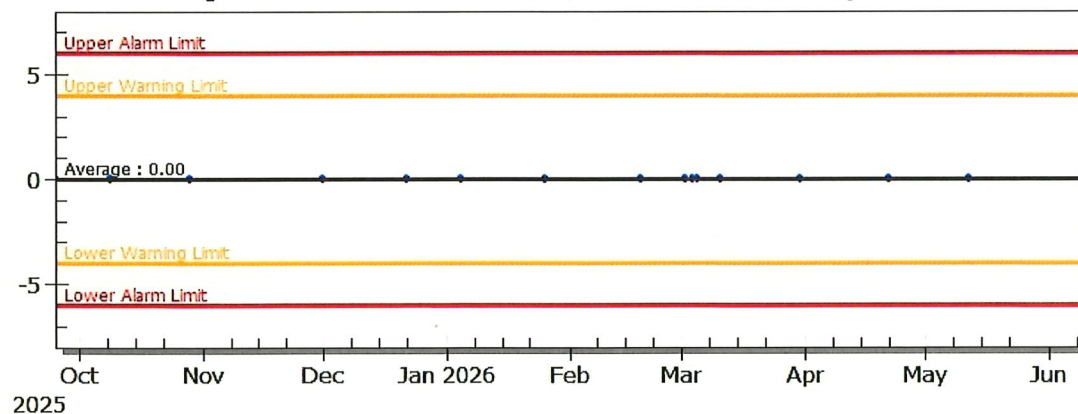


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For HCl from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : HCl

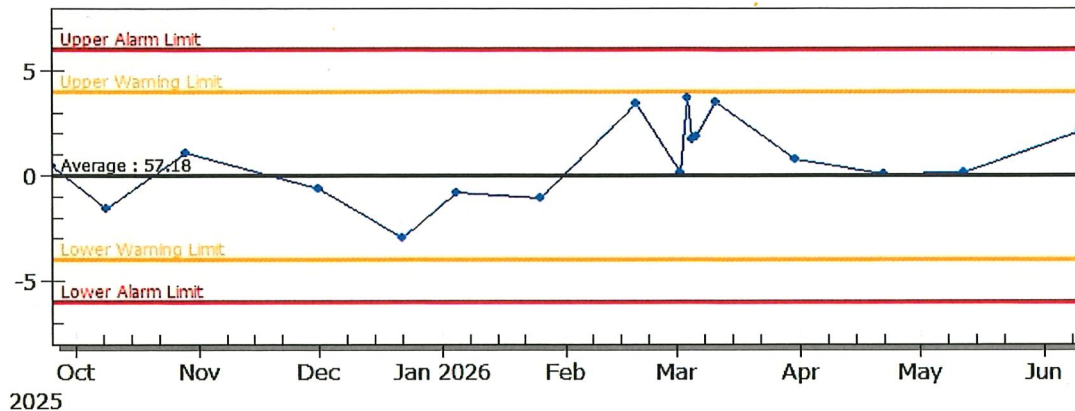

Last Test Date 10/06/2026 - Bottle Name Hydrogen Chloride (New) - Expiry Date 31/10/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : HCl

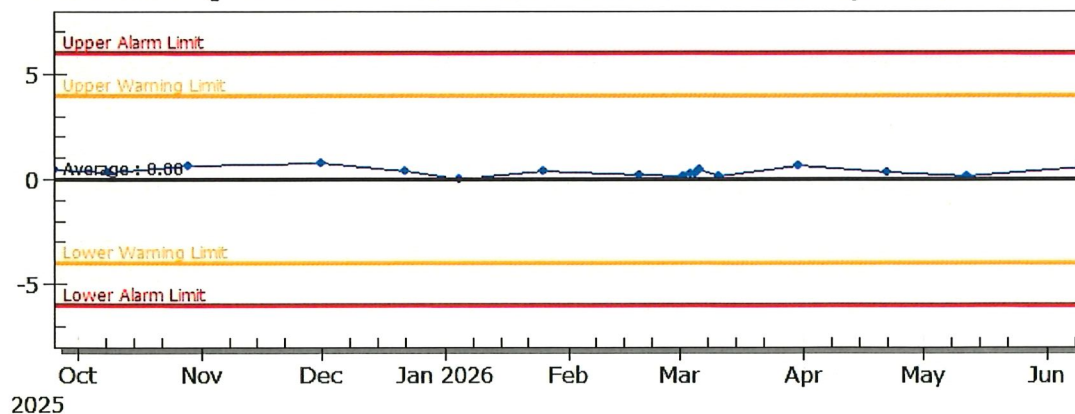


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For N2O from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : N2O

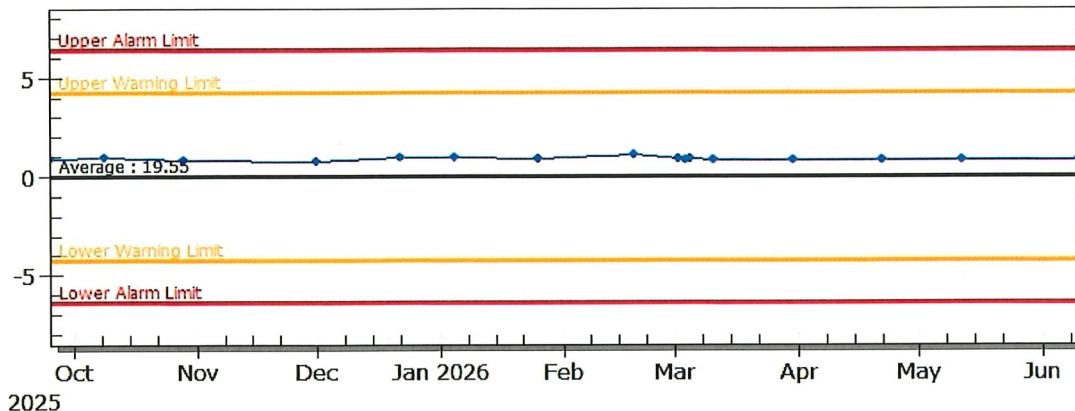

Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : N2O

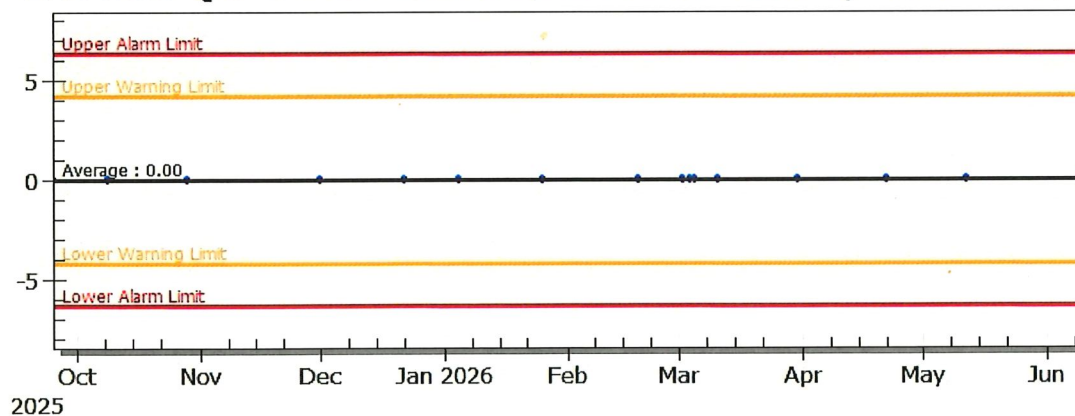


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NH3 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : NH3

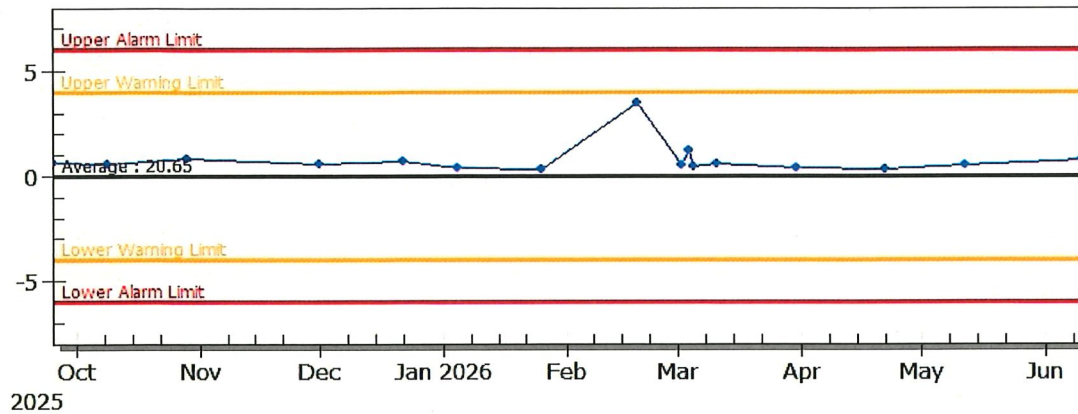

Last Test Date 10/06/2026 - Bottle Name Ammonia - Expiry Date 04/02/2026

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : NH3

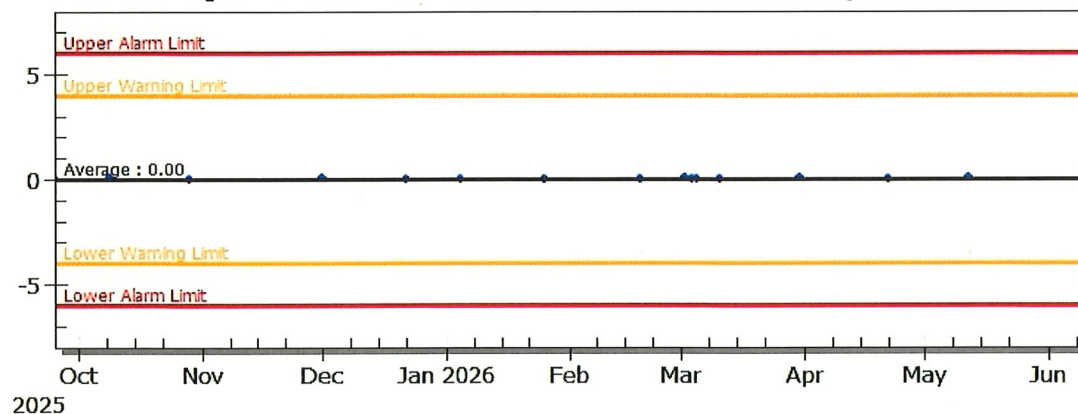


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For NO from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : NO

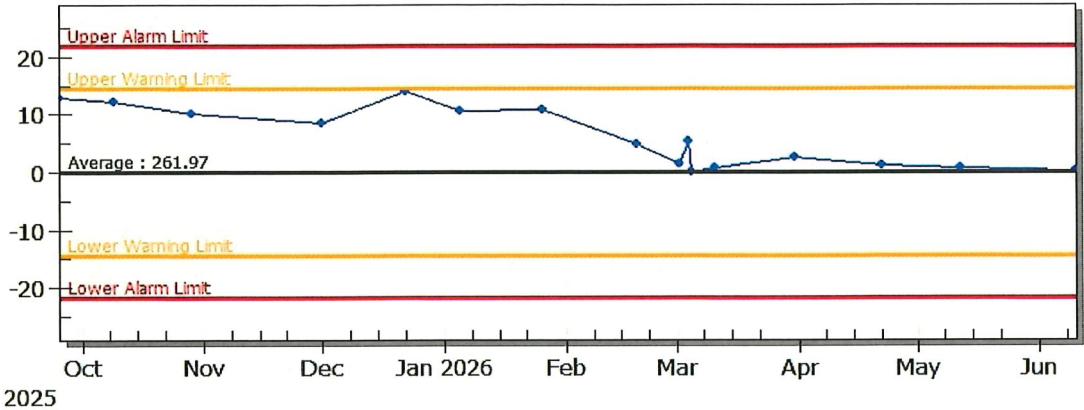

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : NO

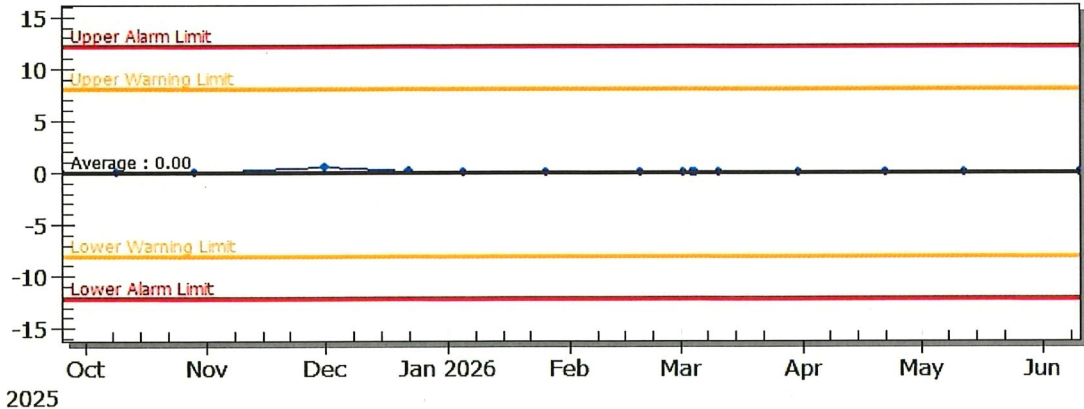


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For O2 from 29 October 2025 to 29 October 2025

EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : O2

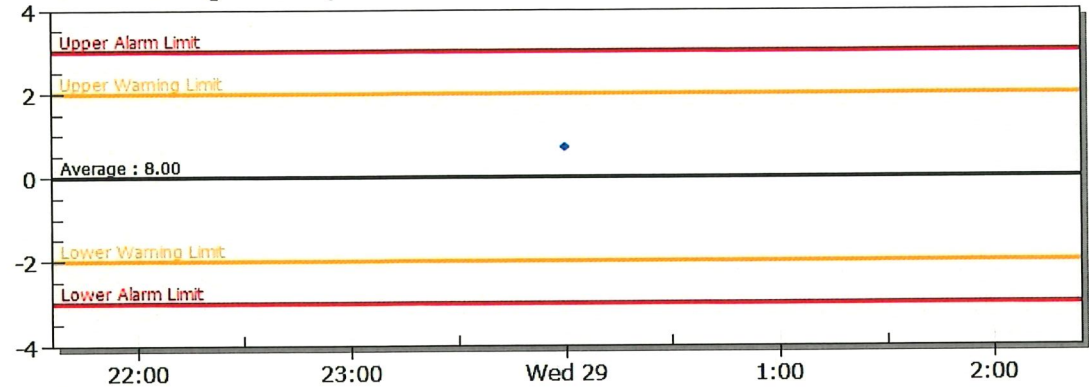


Oct Tue 28 2025

Last Test Date 10/06/2026 - Bottle Name CO2/O2 - Expiry Date 20/12/2027

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : O2

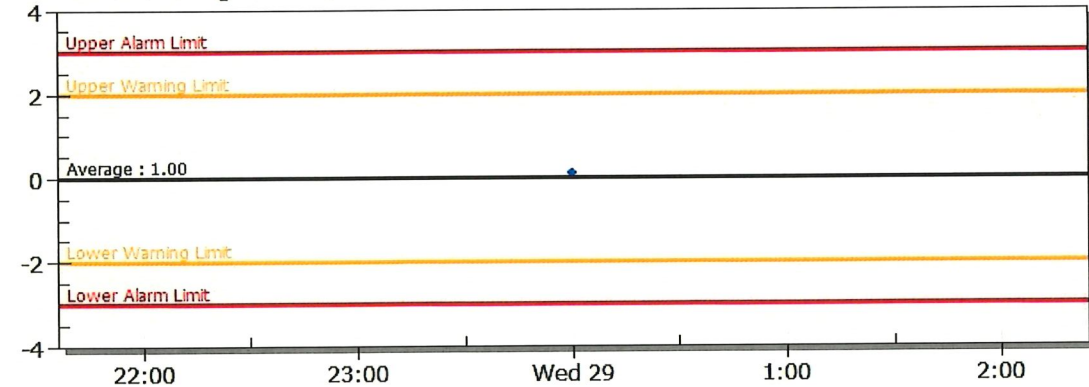


Oct Tue 28 2025

Last Test Date 29/10/2025 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Passed

QAL3 Report For Propane from 25 September 2025 to 10 June 2026

EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : Propane

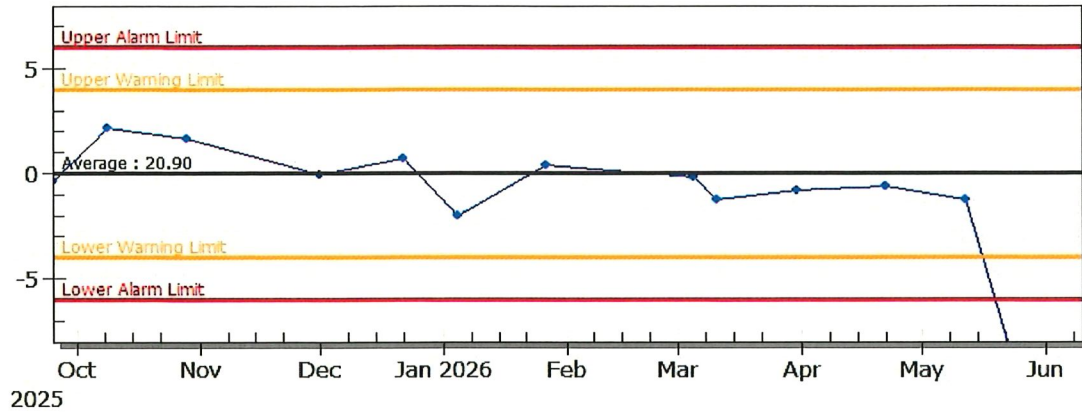


Last Test Date 10/06/2026 - Bottle Name N2O / O2 / Propane - Expiry Date 06/09/2025

Test Has Failures and/or Warnings

Span Test - Single Point Above the Alarm Limit (10 June 2026)

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : Propane

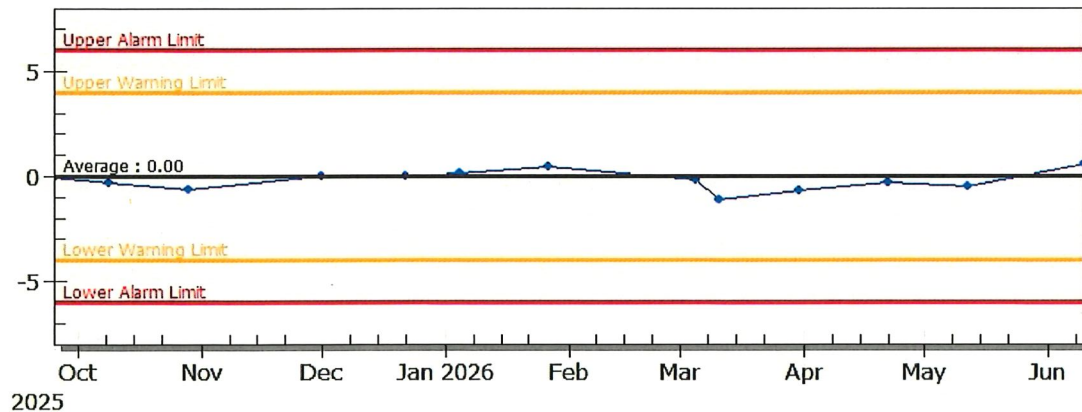


Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed

QAL3 Report For SO2 from 25 September 2025 to 10 June 2026


EN14181 QAL 3 Span Shewhart Chart for Standby MIRFT : SO2

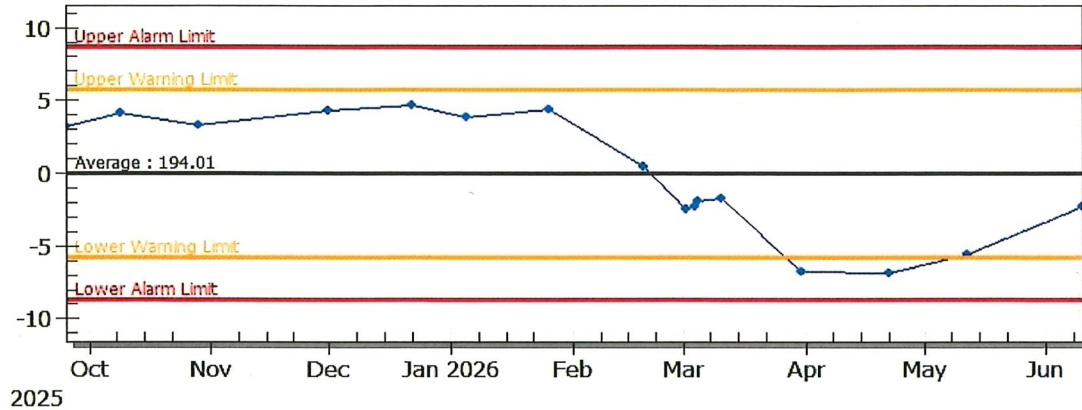

Last Test Date 10/06/2026 - Bottle Name CO/SO2/NO - Expiry Date 15/08/2028

Test Passed

EN14181 QAL 3 Zero Shewhart Chart for Standby MIRFT : SO2

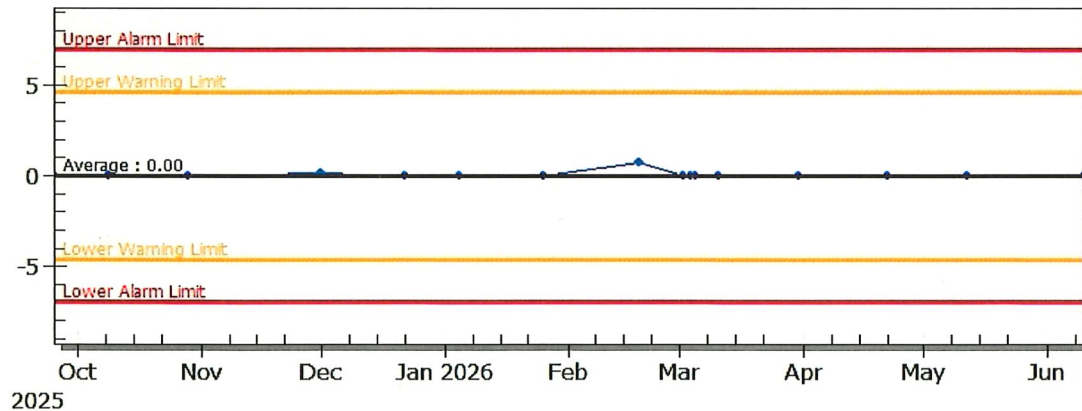

Last Test Date 10/06/2026 - Bottle Name Nitrogen - Expiry Date 25/12/2030

Test Passed